

LAPORAN HASIL UJI

Contoh uji diajukan dan diidentifikasi oleh pelanggan sebagai berikut:

APLIKAN / PEMOHON	: PT. HABITURA PRIMA NAWASENA
ALAMAT	: JL. CUT MUTIA NO.30 KEL. MARGAHAYU, KEC. BEKASI TIMUR JAWA BARAT 17113
NAMA SAMPEL	: AVS FIBERGLASS SILRUB 1715/2
JENIS PENGUJIAN	: UJI TARIK REGANGAN UJI BAKAR
STANDAR	: ASTM D 638-22 SNI 0989:2011
CONTOH DITERIMA	: 16 Juni 2025
CONTOH DIUJI	: 16 Juni 2025
KETERANGAN	: Lihat Lembar Lampiran

Lampiran yang ada merupakan bagian yang tidak terpisahkan dari sertifikat ini.

Hasil uji ini hanya terkait dengan contoh uji yang diserahkan saat itu saja dan laporan / sertifikat hasil uji tidak dapat di produksi dengan cara apapun, kecuali dalam konteks penuh dengan persetujuan tertulis sebelumnya dari Laboratorium Sucofindo Penerbitan Sertifikat/Laporan ini tunduk pada Syarat dan ketentuan Umum layanan jasa PT. SUCOFINDO (PERSERO), yang salinannya dapat diperoleh atas permintaan atau dapat diakses pada www.sucofindo.co.id



38010625001097

Sub Bagian Teknik

Fandi Firmadi



5260784



SCI-2023A

LAPORAN HASIL UJI

Nama Sampel : AVS FIBERGLASS SILRUB 1715/2

 Kondisi Pengujian
 - Temperatur : 23.2°C
 - Kelembaban : 54%

Diuji oleh : Hendri Sukrisno

Diverifikasi oleh : Lukman Prasetyo


 Peralatan Uji : - Universal Testing Machine
 S/N AP90911
 - Flammability Tester
 S/N 13359

Disetujui oleh : Fandi Fermadi



No	Item Pengujian	Unit	Hasil
1.	Uji Tarik	N/mm ²	106.17
	Regangan	%	2.8
2.	Uji bakar	-	Kelas 1 (DNI)


DNI = Do Not Ignite (Tidak Terbakar)

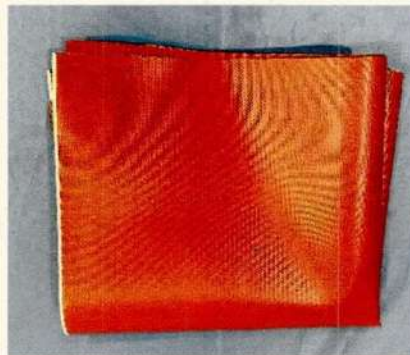

Gambar Sampel



Gambar Pengujian

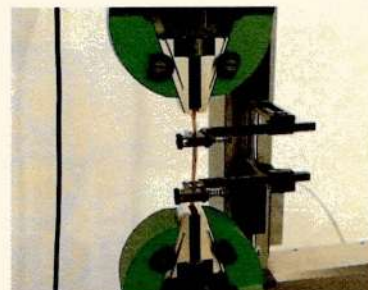

Gambar Pengujian



CALIBRATION CERTIFICATE**SERTIFIKAT KALIBRASI**

(No : 1672-1/EKI/XII/2025)

Ship's Name : - Job Title : -
Nama Kapal : - Jabatan : -

Owner Name : PT. HABITURA PRIMA Address : Jl. Cut Mutia No.30 Kel. Margahayu,
Nama Pemilik : NAWASENA Alamat : Kec. Bekasi Timur Kota Bekasi, Jawa Barat 17113

Phone no. : - Fax No. : - Email :
No. Telp : - No. Faks : -

Instrument Identity

Identitas Instrumen

Name : Fixed Gas Detector
Nama : H₂S

Serial Number : M02SJ087
Nomor Seri

Manufacturer : Henan Inte
Merk Pabrik : KQ-500D H₂S

Standard Identity

Identitas Standar

Name : Standard Gas Mixtures
Expired Date : 2026
GAS COMPOSITION Lot : 30441213450-1
METHANE : 2,5% (50% LEL)
HYDROGEN SULFIDE : 25 ppm
OXYGEN : 18 % vol
CARBON MONOXIDE : 100 ppm
NITROGEN : Balance

Environmental Condition During Calibration

Kondisi Lingkungan Selama Kalibrasi

Date of Acceptance : December 24, 2025
Tanggal Penerimaan

Date of Calibration : December 25, 2025
Tanggal Kalibrasi

Place of Calibration : In Lab
Tempat Kalibrasi

Calibration Method : Direct Comparison to
Metode Kalibrasi : Certified Gas

Relative Humidity : 55.6 ± 6.4 % RH
Kelembaban Relatif

Temperature : 25.2 ± 4.2 °C
Suhu

Traceability : to SI Units through Calgaz
Ketertelusuran : Minor



HO
Gedung 18 office park, lantai 25
suite A2, jl tb simatupang kav 18,
kel. Kebagusan kec. Pasar minggu,
jakarta selatan 12520



Lab &
Workshop PT Efusi Laboratorium Prima
Jalan Naming D Bothin. RT 008 RW.019
Depok Pancoran Mas, Kota Depok
Jawa Barat 16431

LK-430-IDN



AIR FUSION GAS SYSTEM

+62 21 77812874
+62 813 1562 8738
info@kalibrasidulu.co.id
www.kalibrasidulu.co.id

CALIBRATION CERTIFICATE**SERTIFIKAT KALIBRASI**

(No : 1672-1/EKI/XII/2025)

CALIBRATION RESULT**HASIL KALIBRASI**

Calibrated On : December 25, 2025
Device : Fixed Gas Detector H₂S
Device maker / model : Henan Inte / KQ-500D H₂S
Serial Number : M02SJ087

Reference Gas	Concentration Value	Unit	Device Reading Unit Under Test (UUT)		
			Unit as received	After calibration	Uncertainty* (±)
HYDROGEN SULFIDE	25	ppm	27	25	1,42

• Results related only to calibrated items

* With confidence level 95% & coverage factor (k) = 2

THIS UNIT HAS PASSED CALIBRATION

Approved by :

**Toni Kurniawan**

Laboratory Manager

(Date: December 26, 2025)

**HO**Gedung 18 office park, lantai 25
suite A2, jl tb simatupang kav 18,
kel. Kebagusan kec. Pasar minggu,
jakarta selatan 12520**Lab &****Workshop** PT Efusi Laboratorium Prima
Jalan Naming D Bothin. RT 008 RW.019
Depok Pancoran Mas, Kota Depok
Jawa Barat 16431

LK-430-IDN

**AIR FUSION GAS SYSTEM**

☎ +62 21 77812874

☎ +62 813 1562 8738

✉ info@kalibrasidulu.co.id

🌐 www.kalibrasidulu.co.id